

FIG. 1

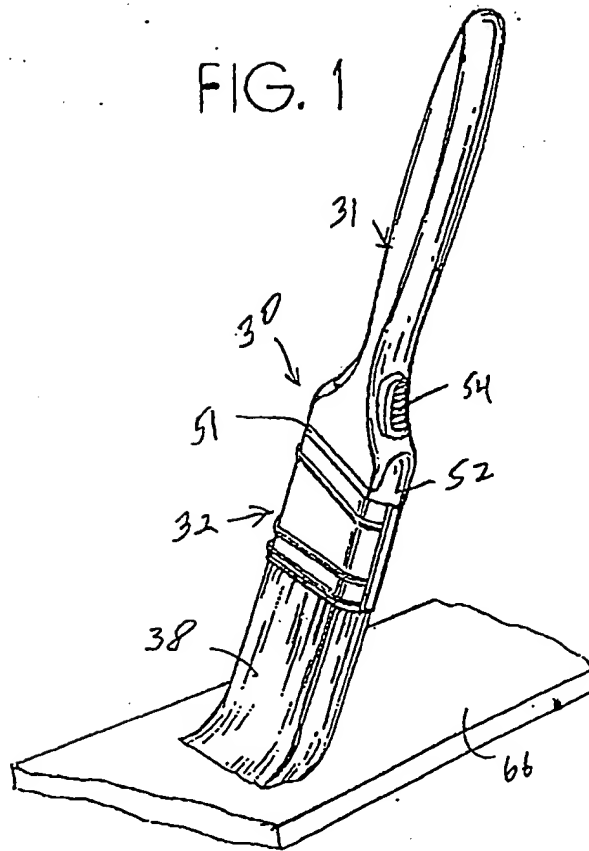
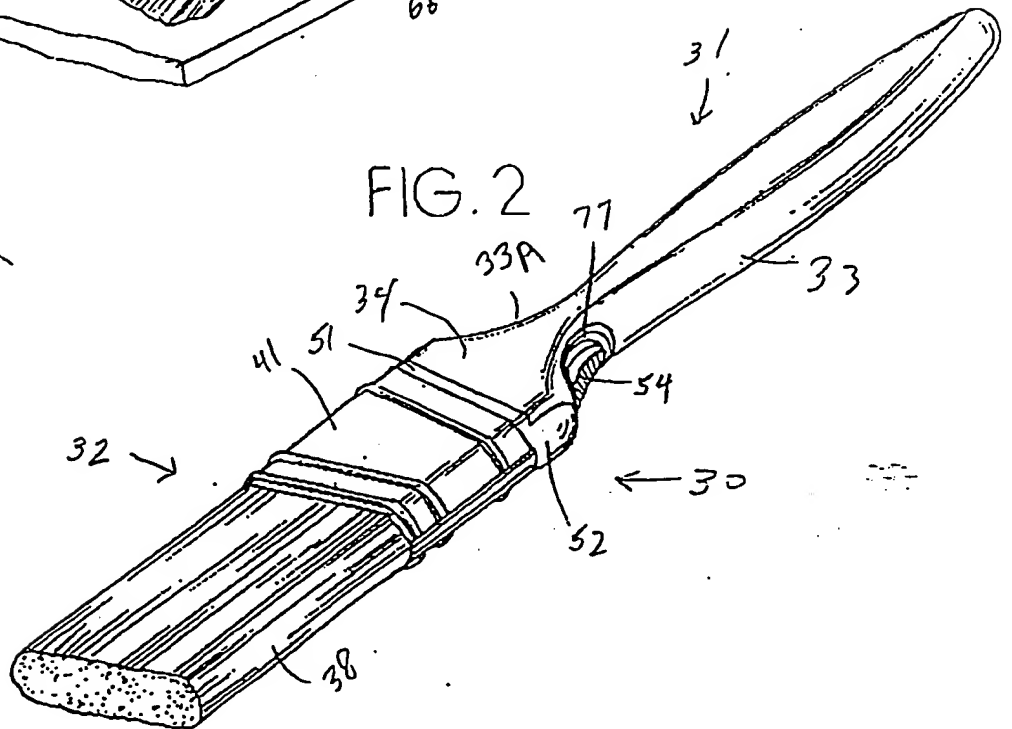
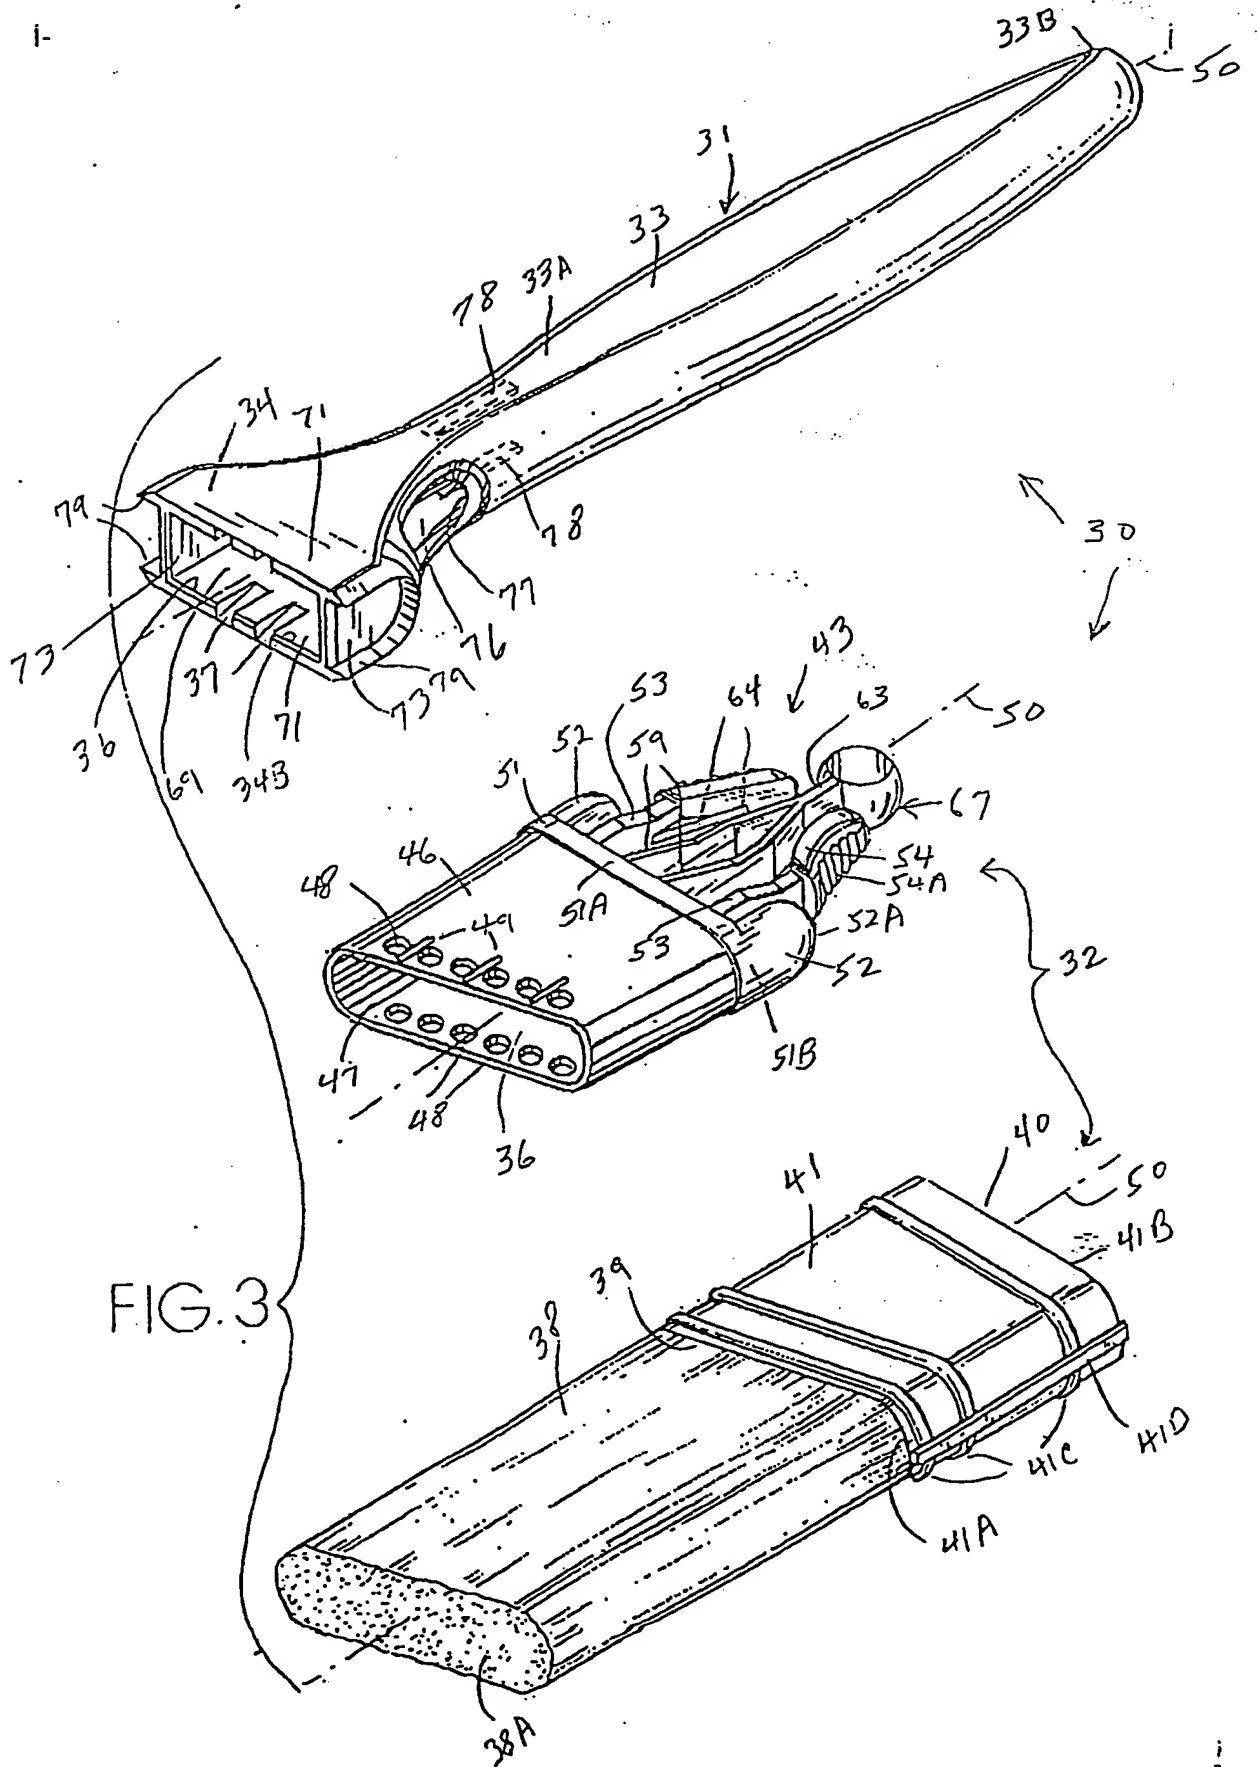


FIG. 2





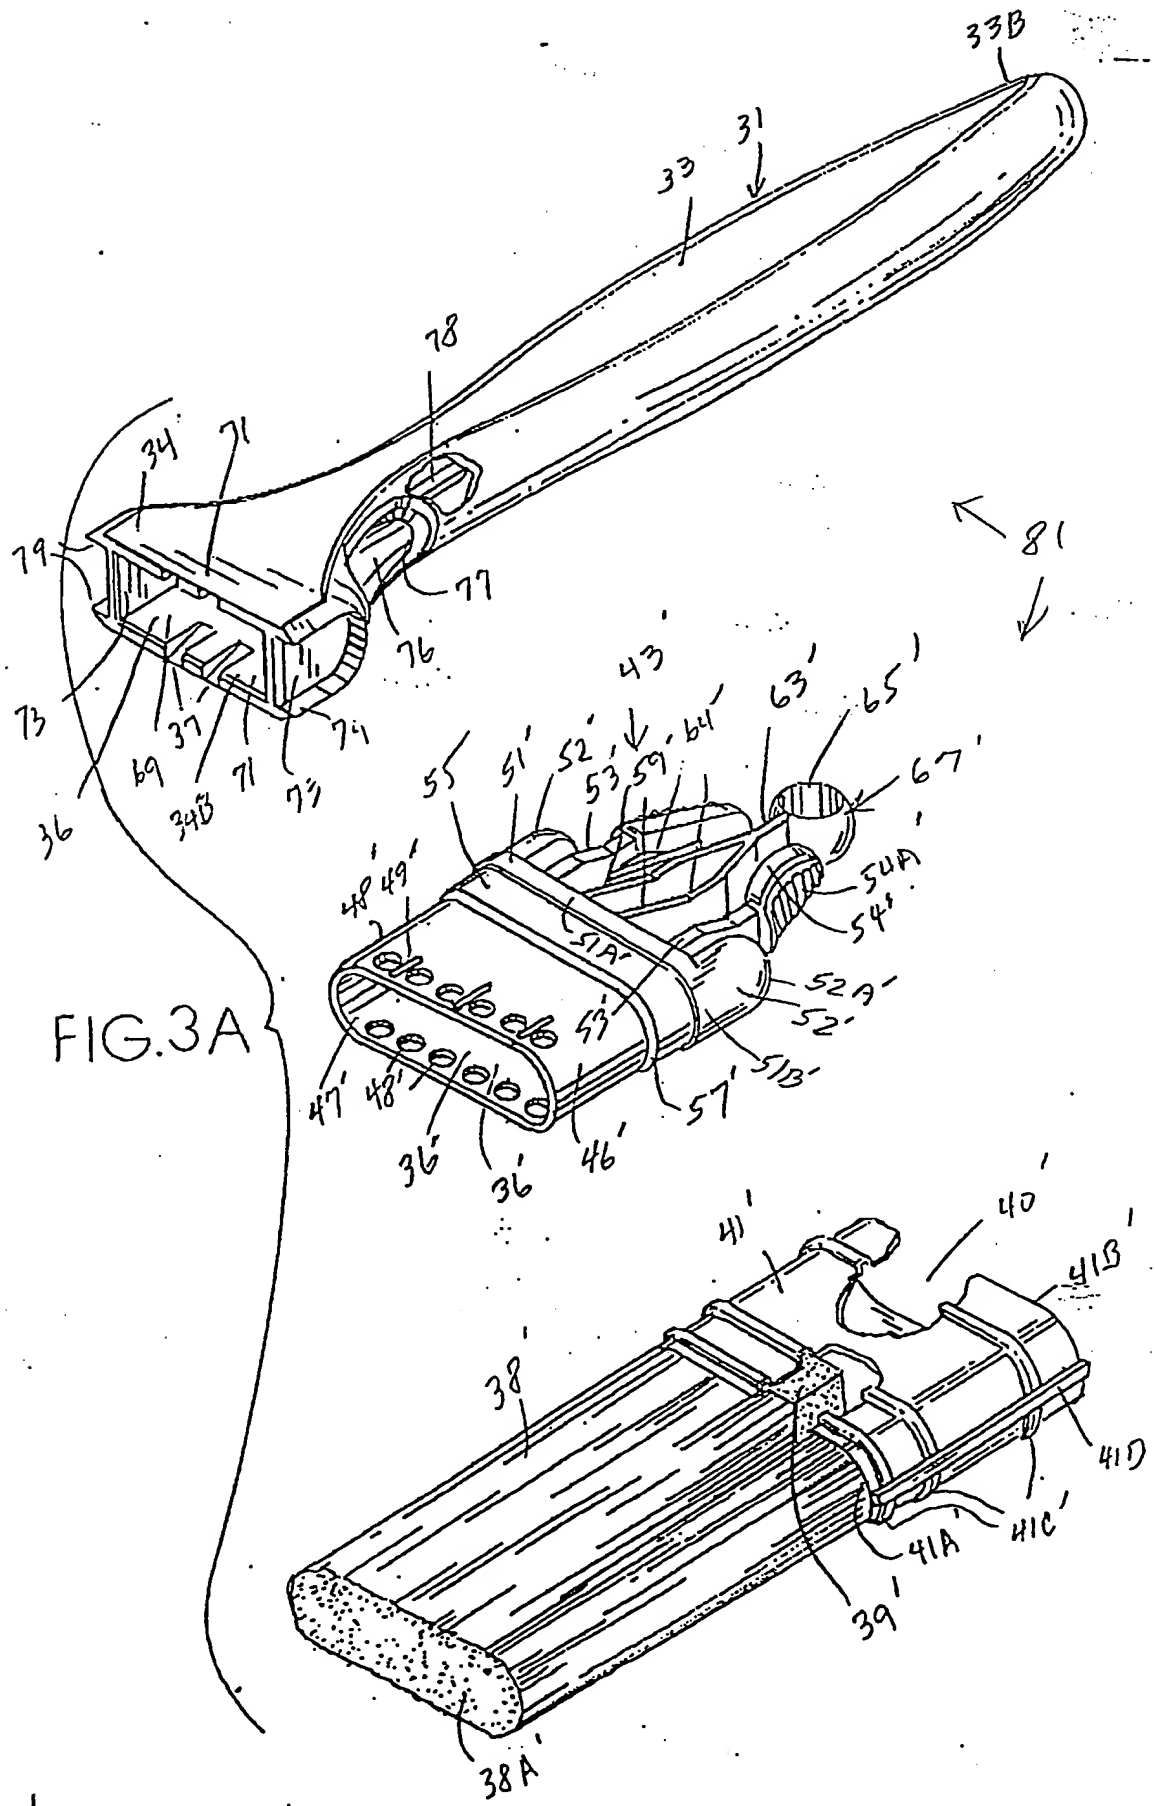


FIG. 4

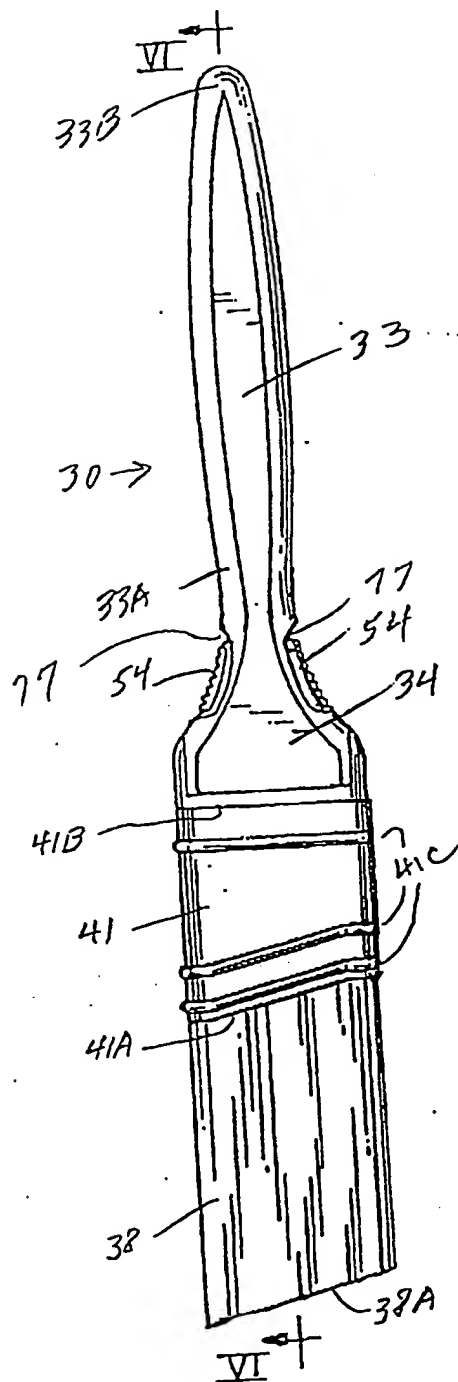


FIG. 5

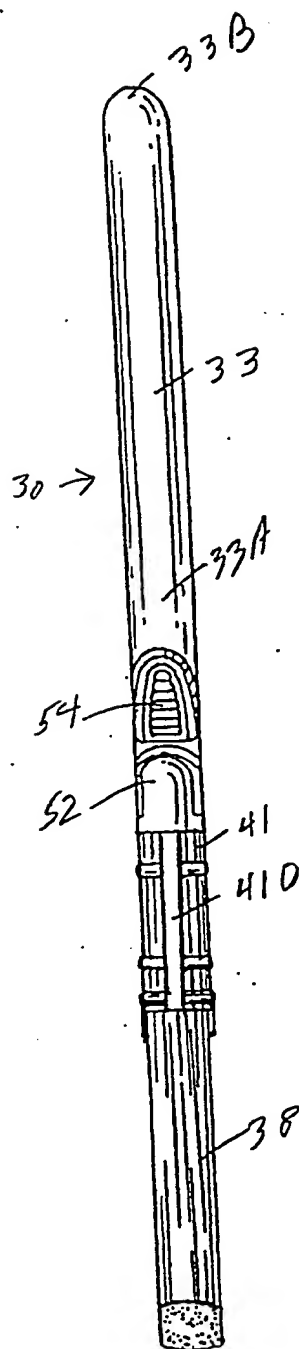


FIG. 6

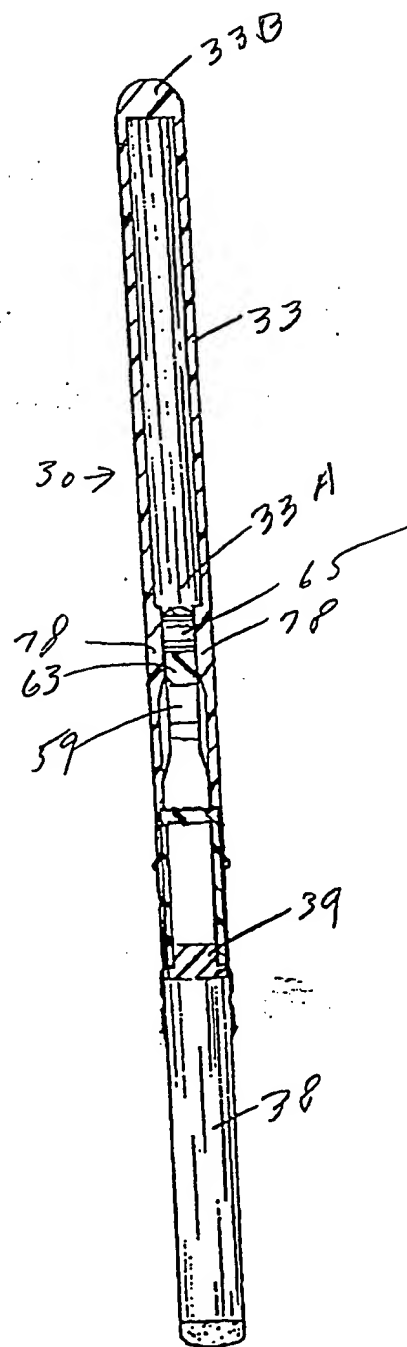


FIG. 7

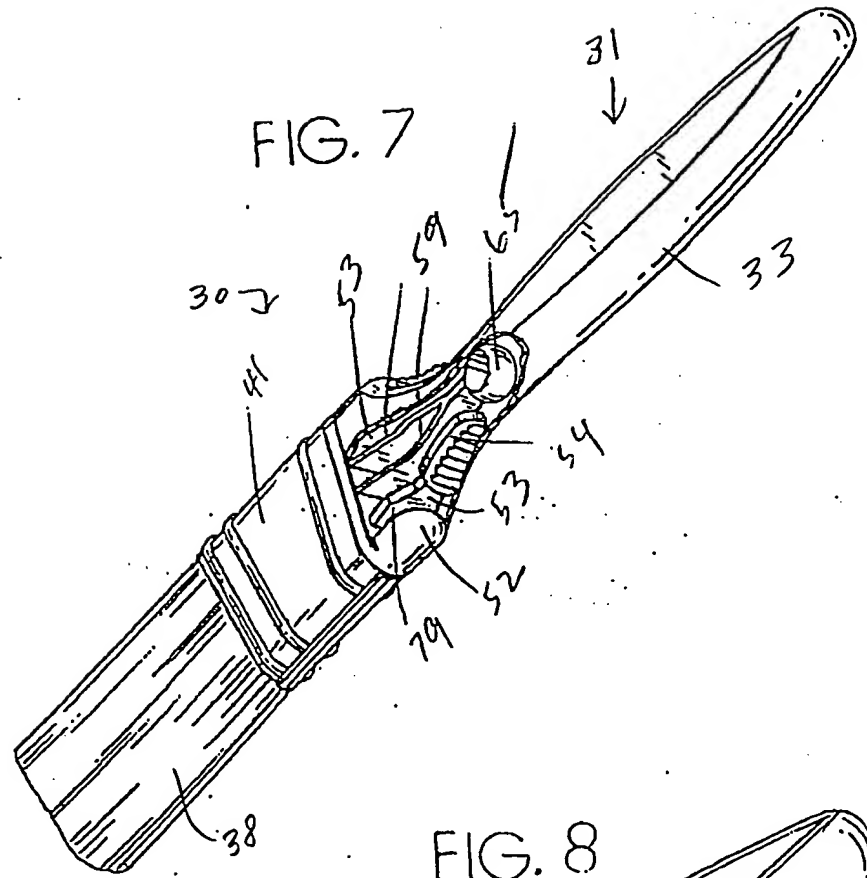
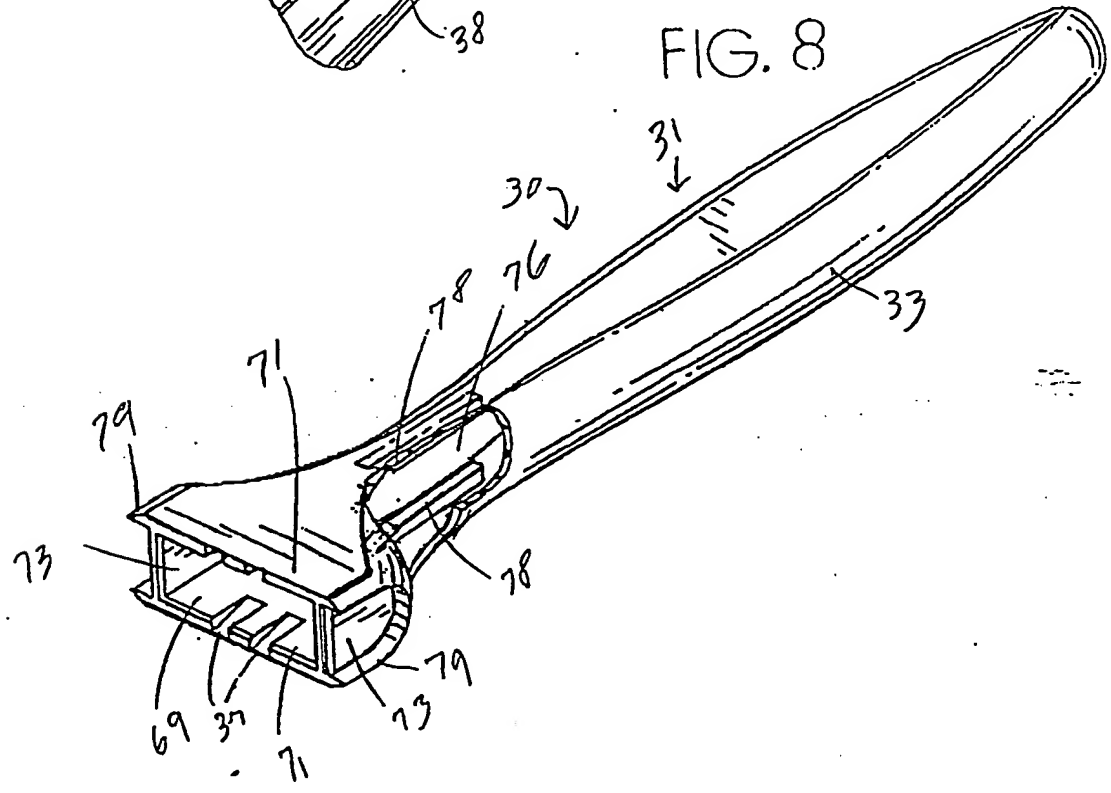
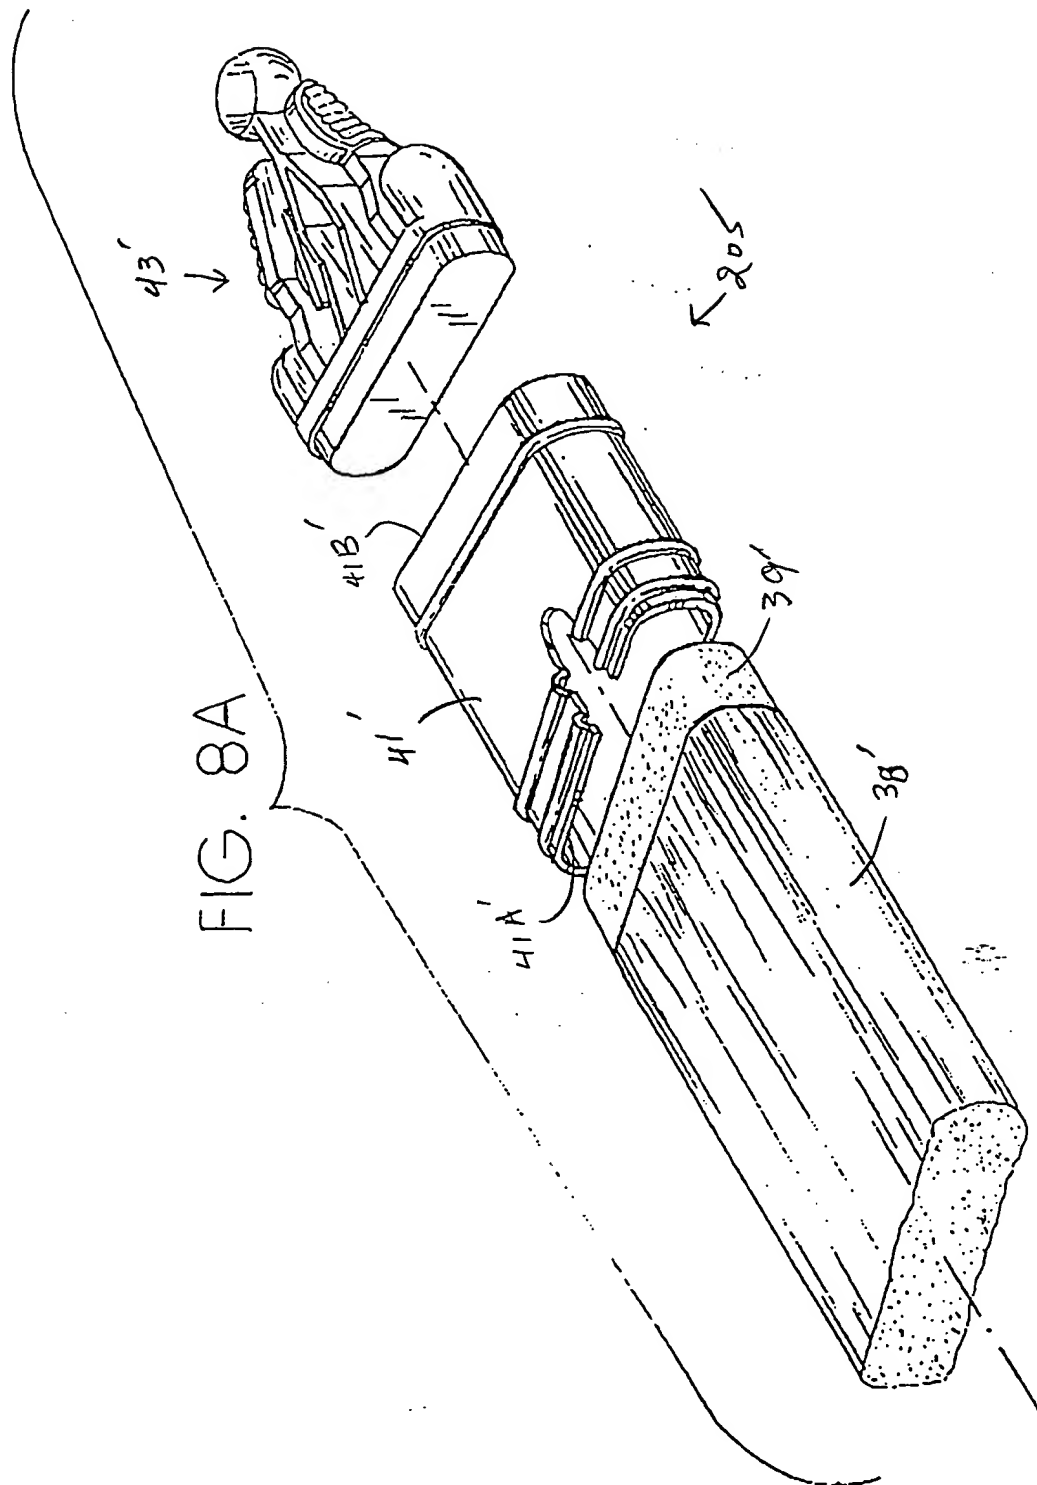


FIG. 8





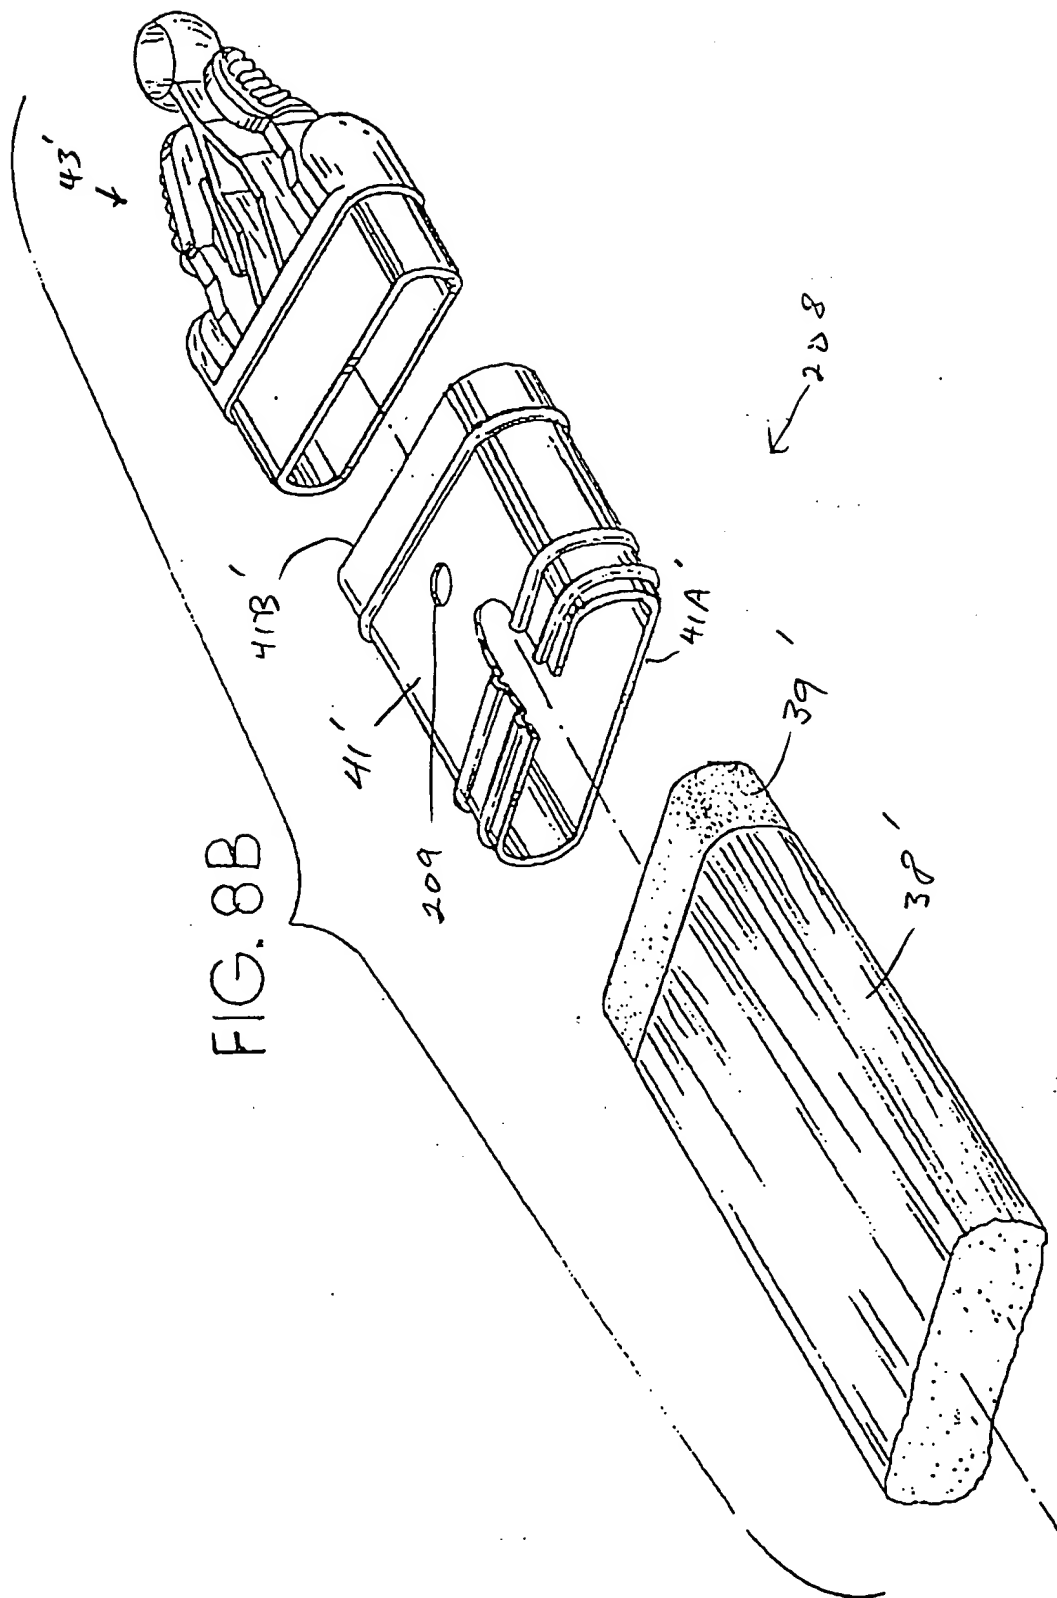
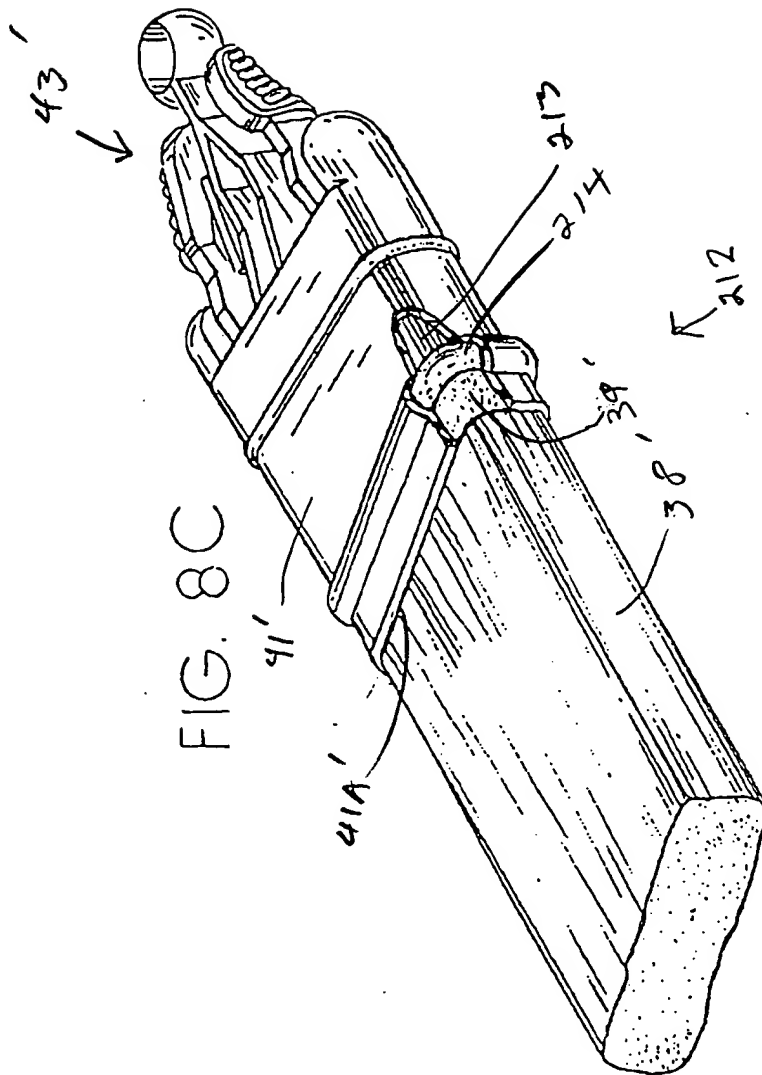


FIG. 8B





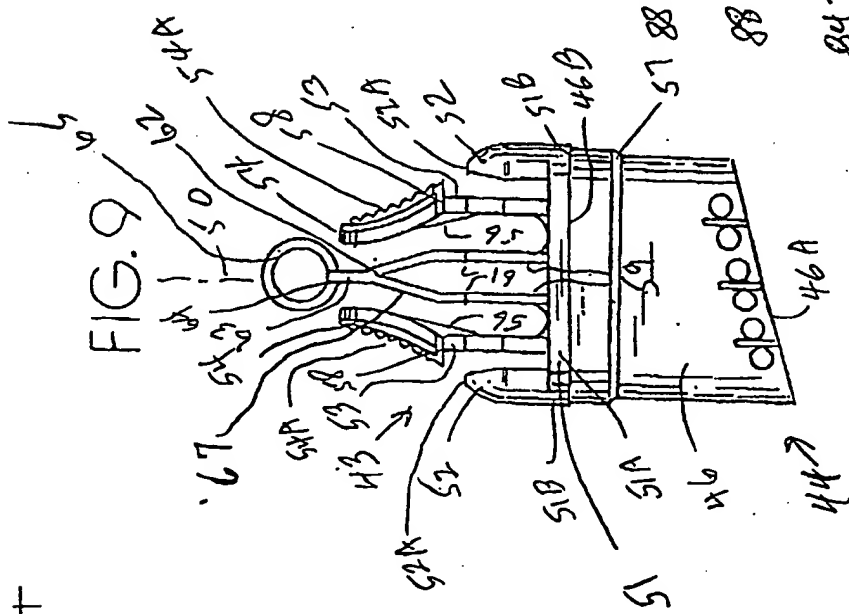


FIG. 12

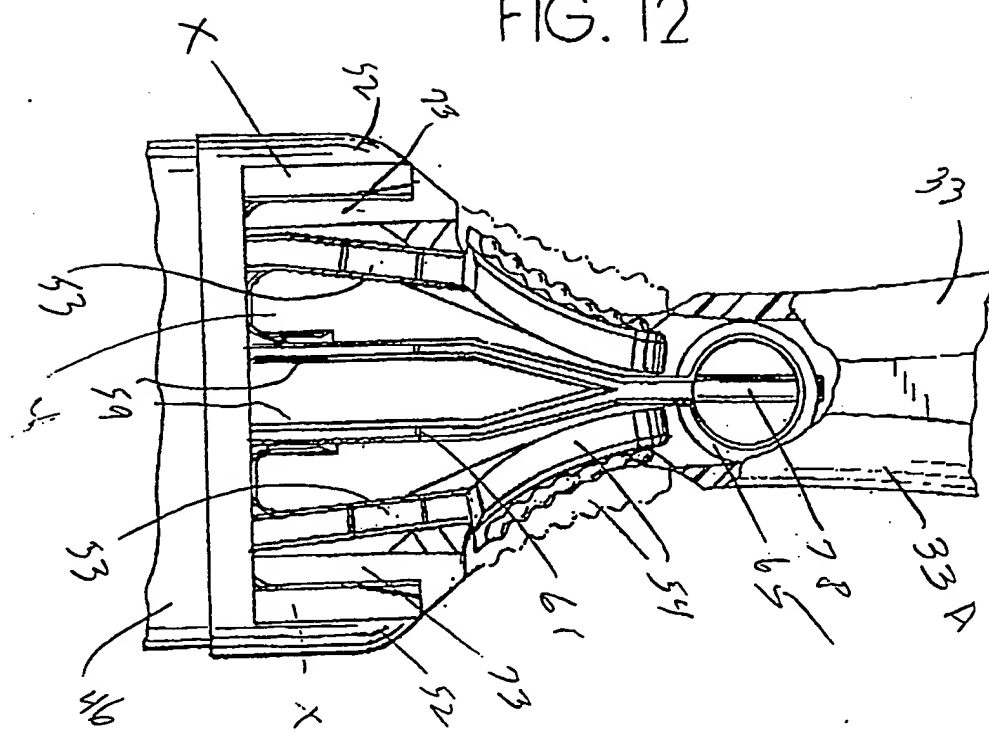


FIG. 13

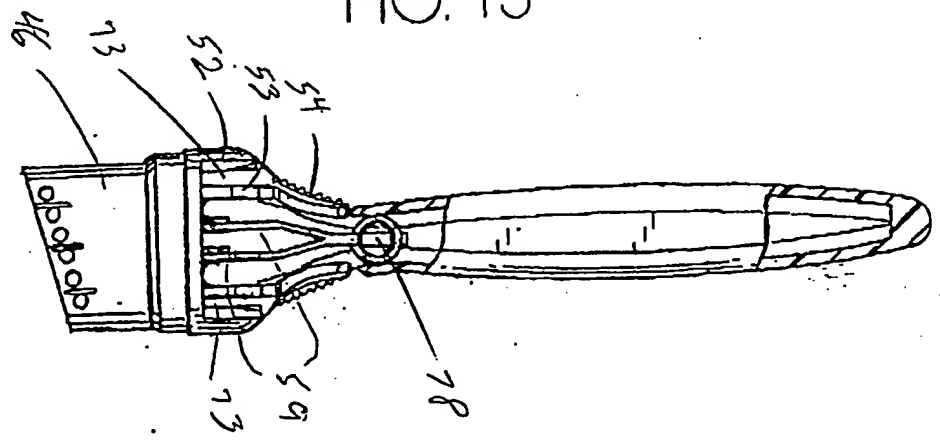


FIG. 12 is a cross-sectional view of the device taken along line X-X of FIG. 13. FIG. 13 is a perspective view of the device.

FIG. 14

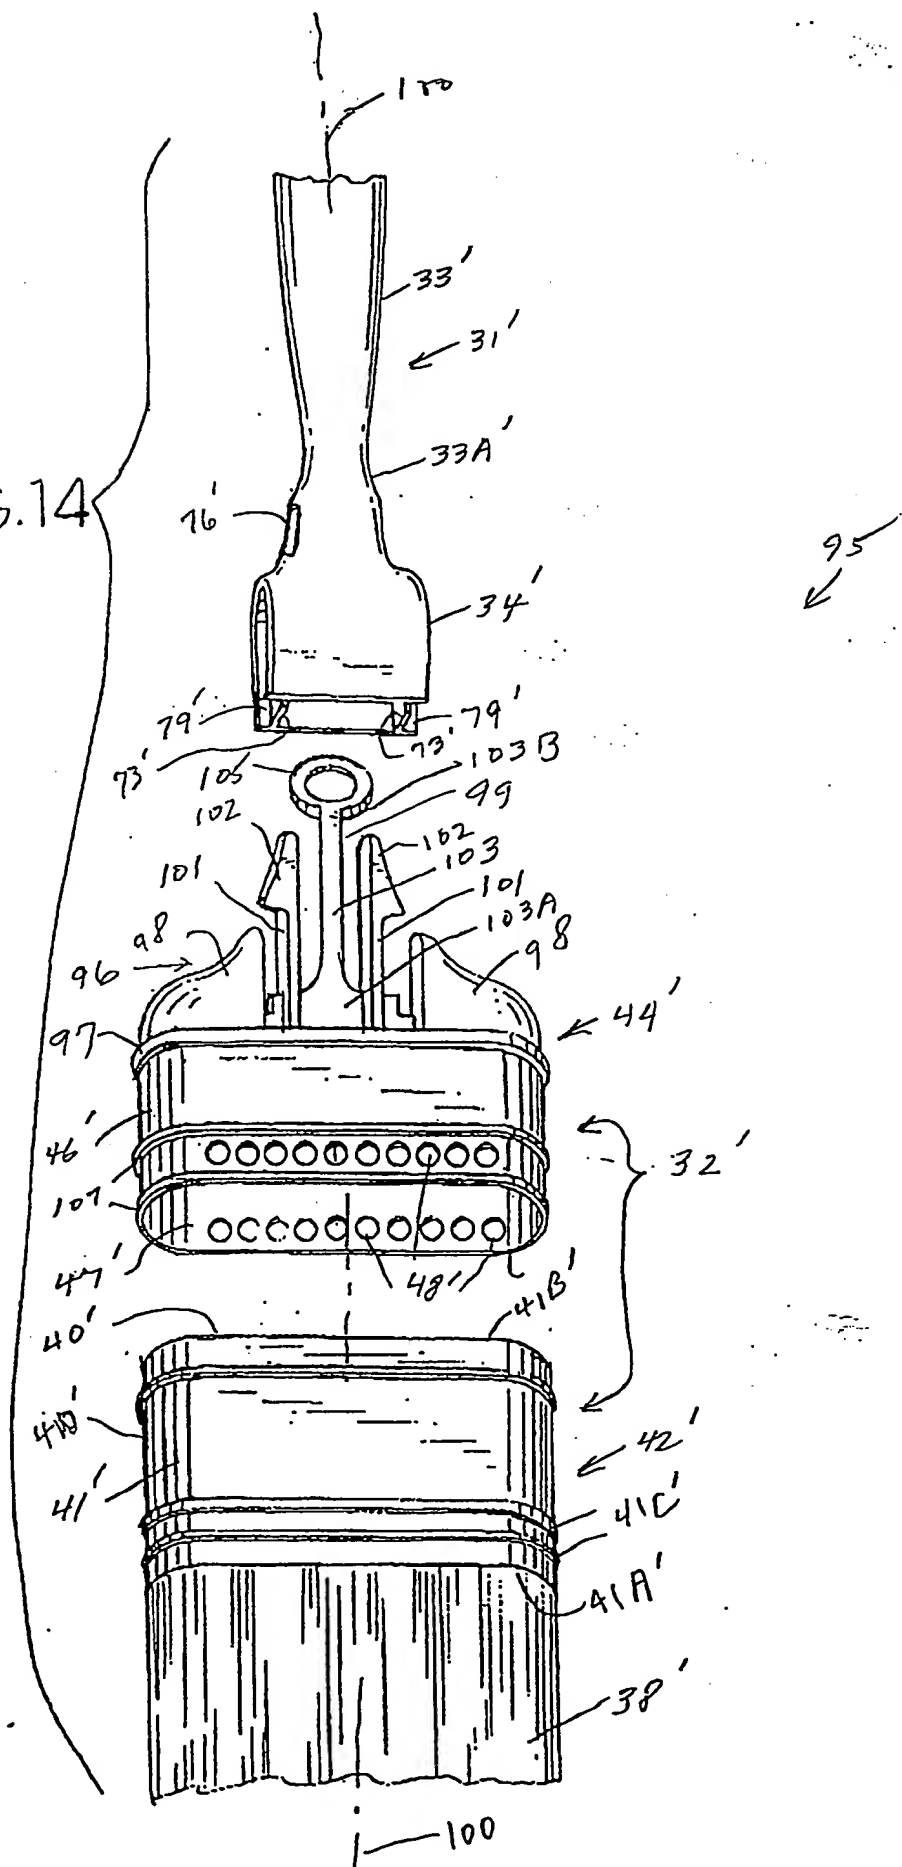


FIG. 15

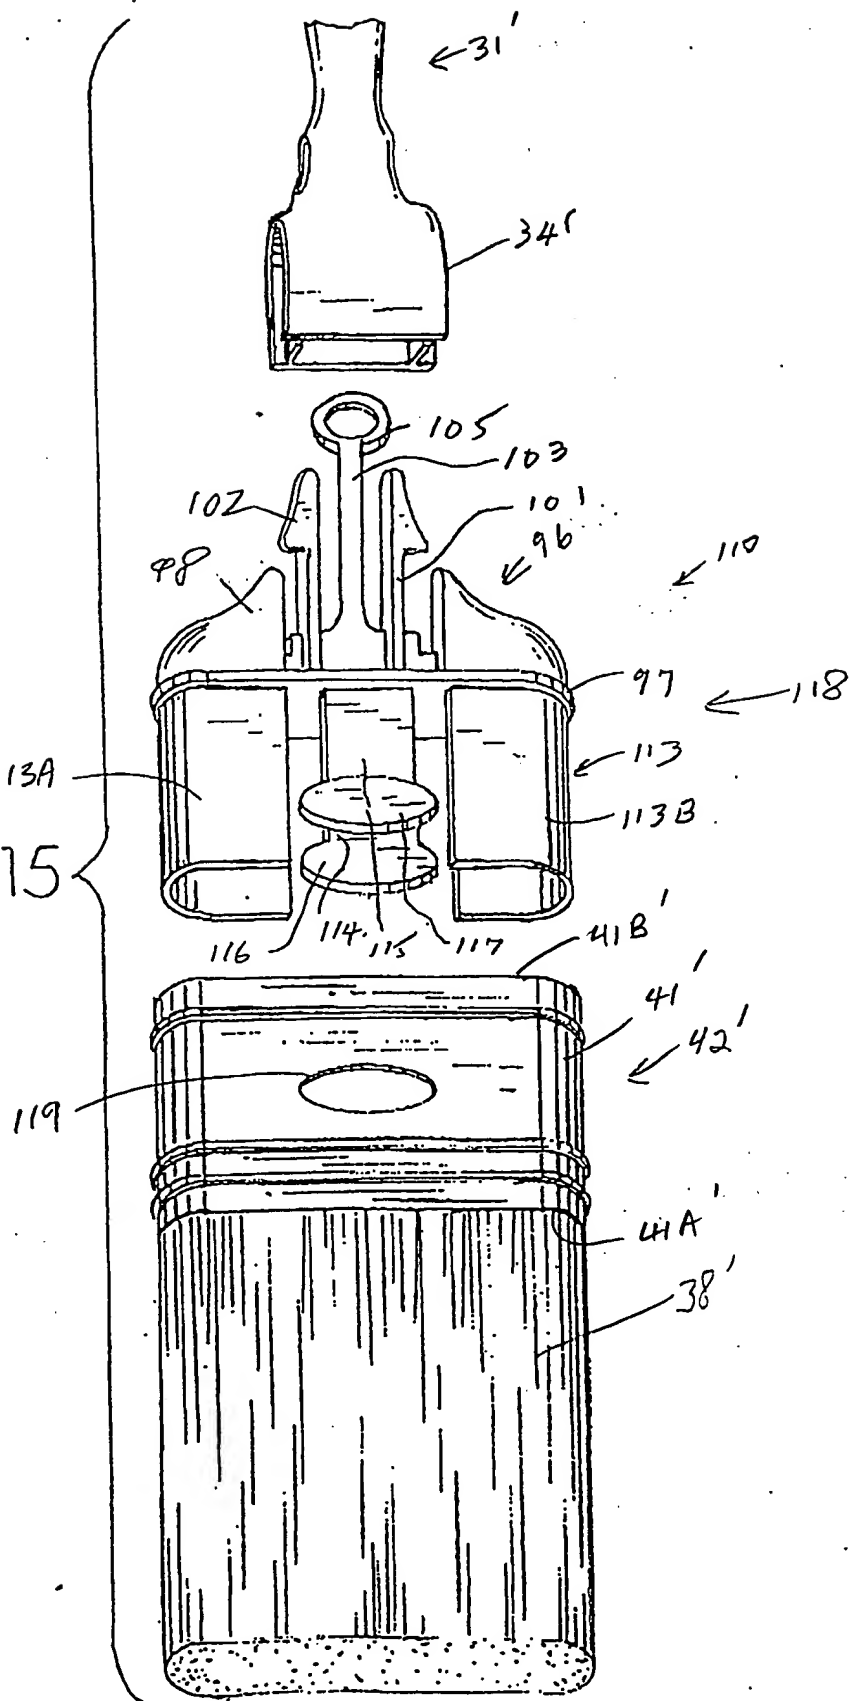
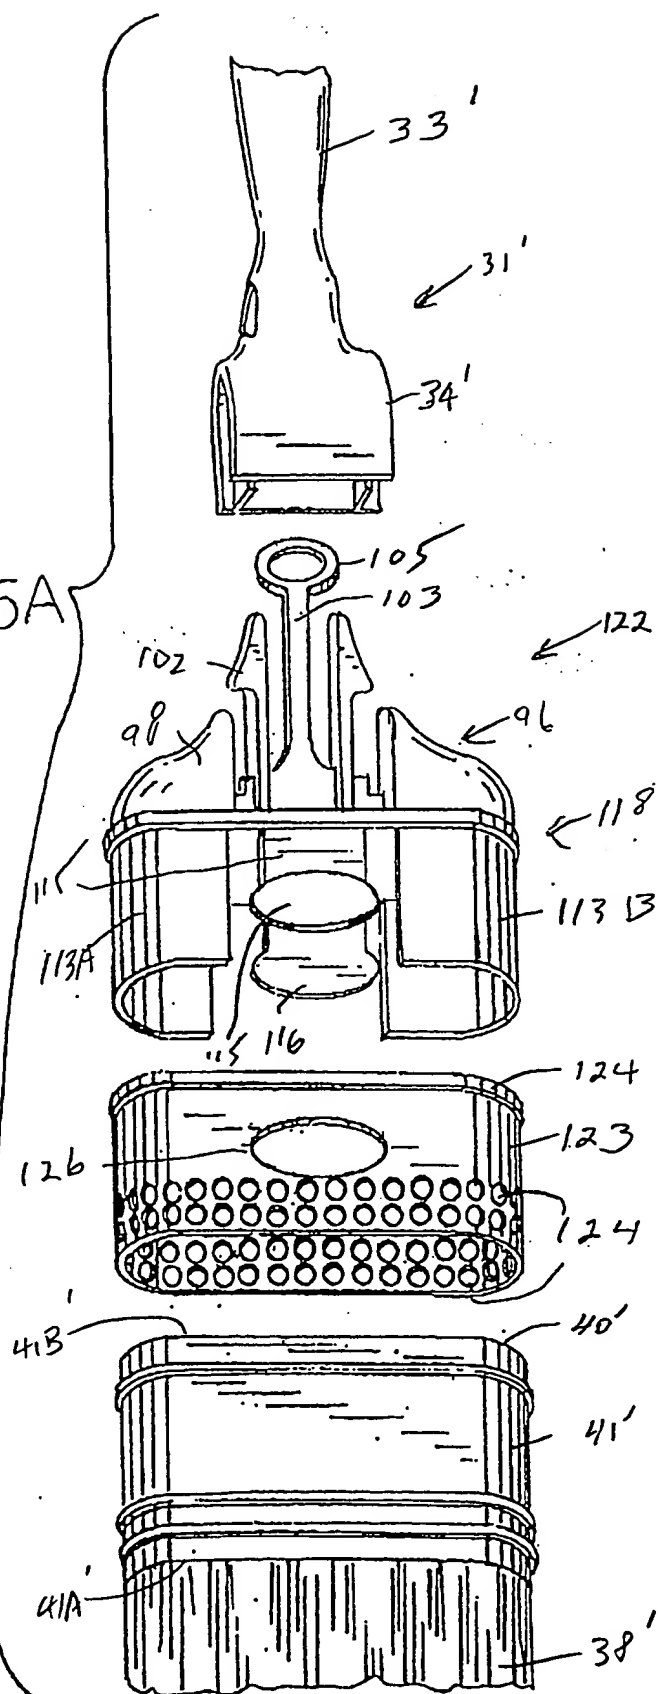
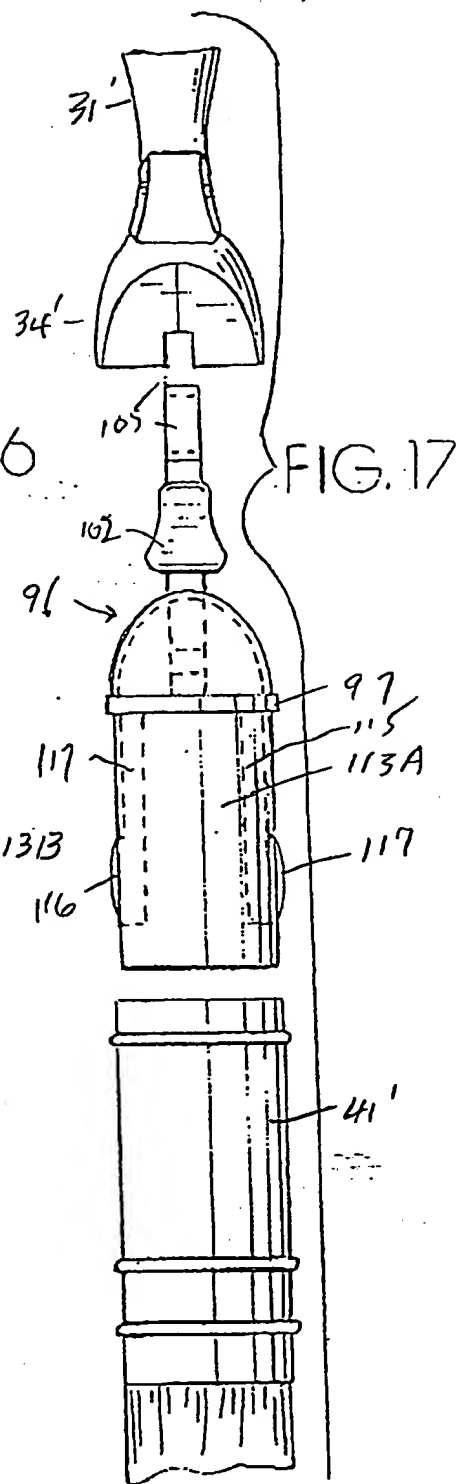
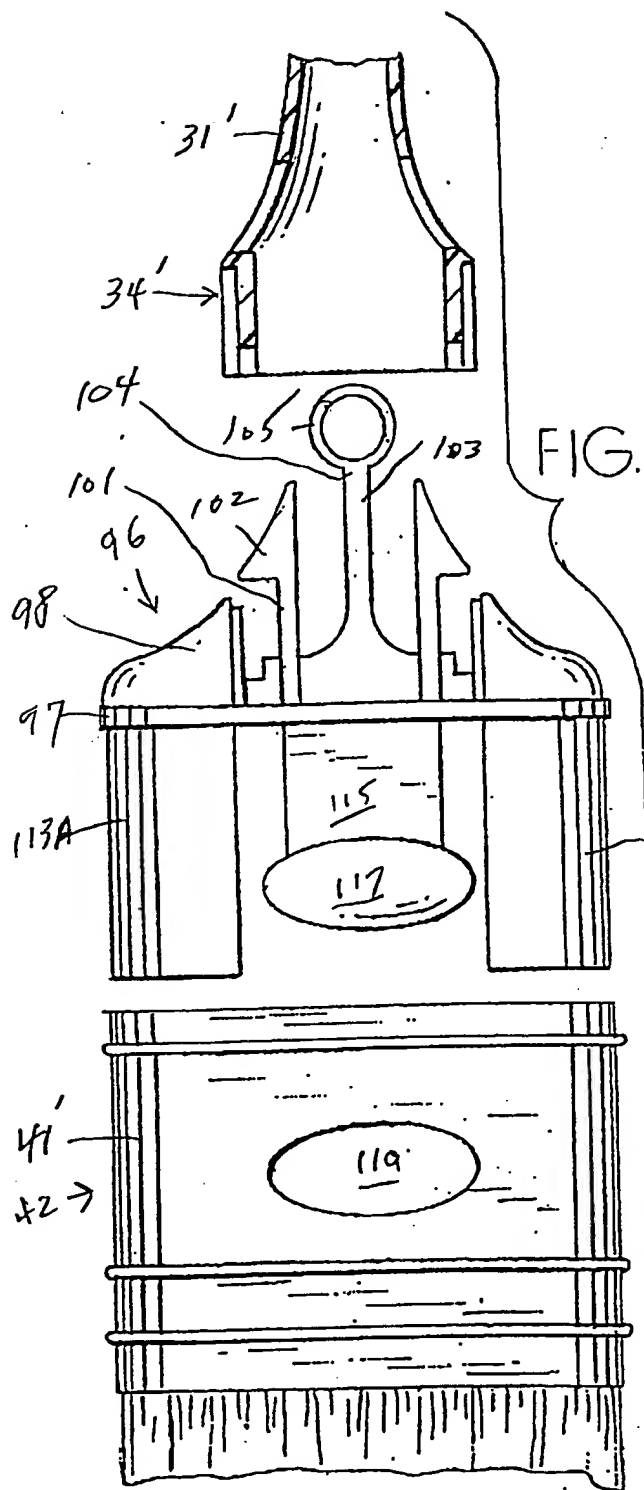


FIG. 15A





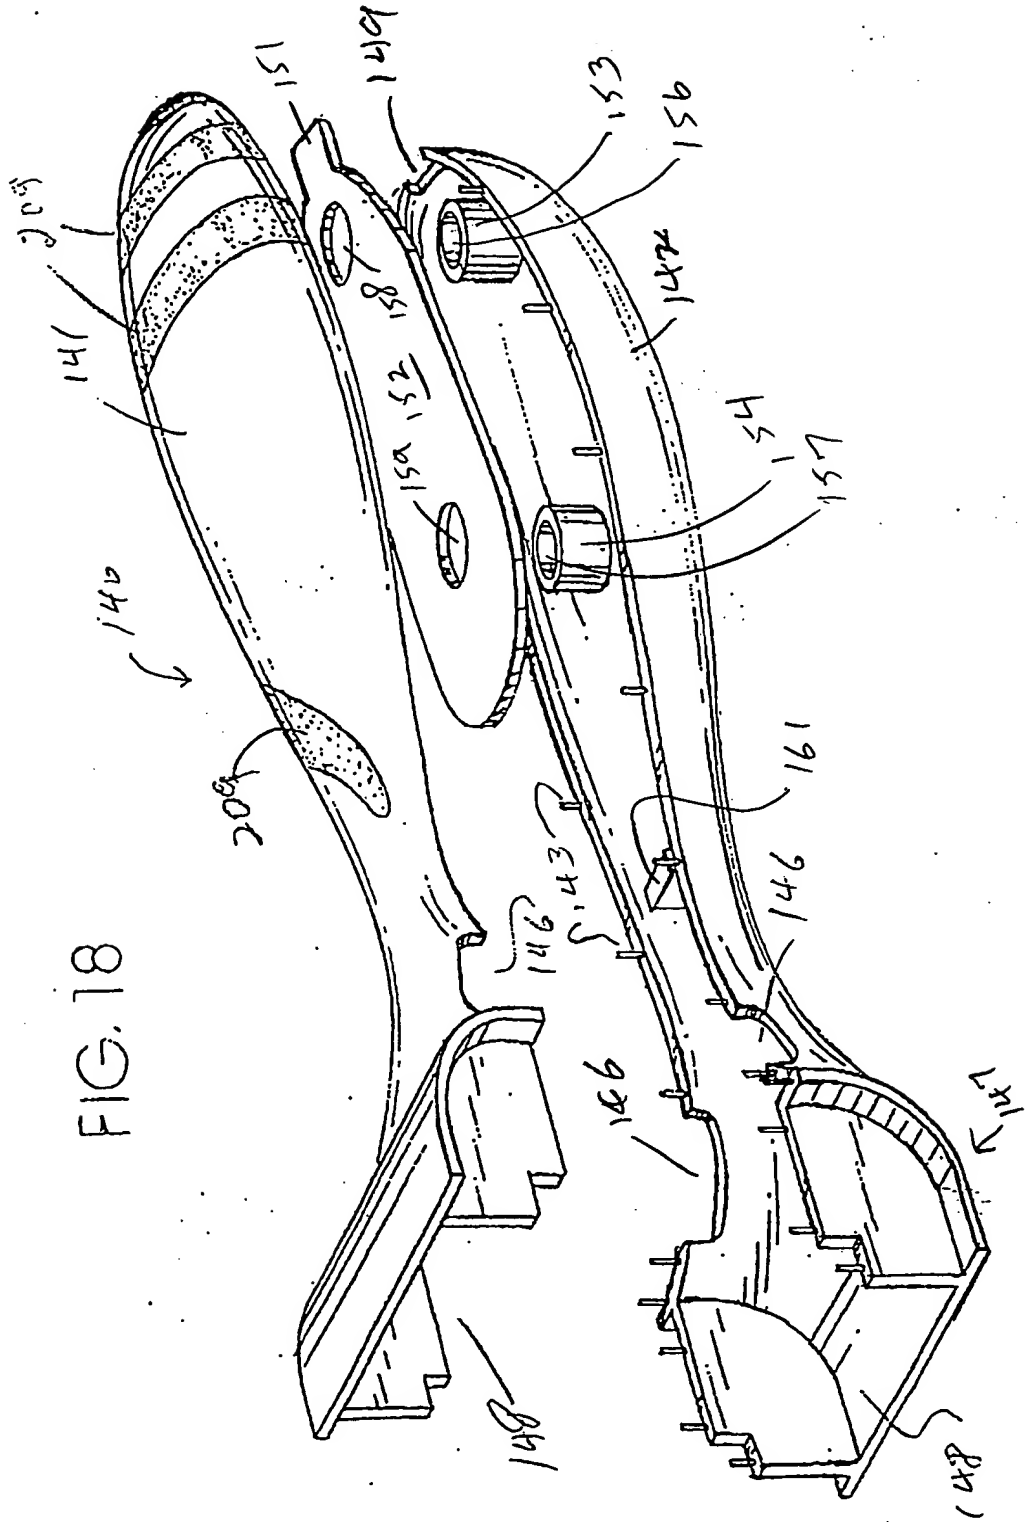


FIG. 19




FIG. 23




FIG. 20A

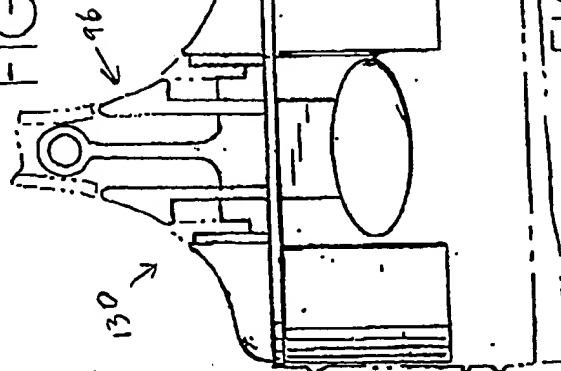


FIG. 20B

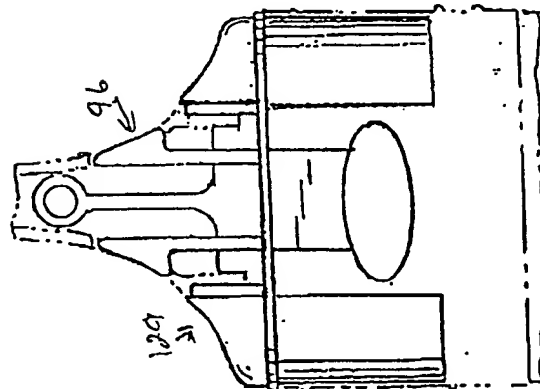


FIG. 20C

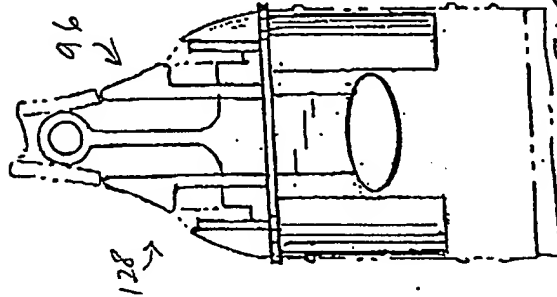


FIG. 22

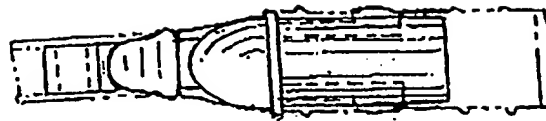


FIG. 21A

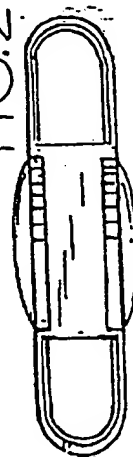








FIG. 21B



FIG. 21C





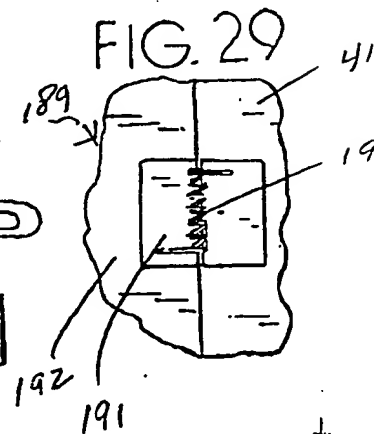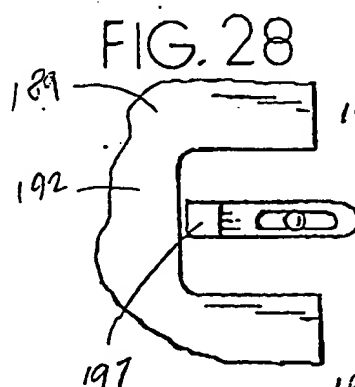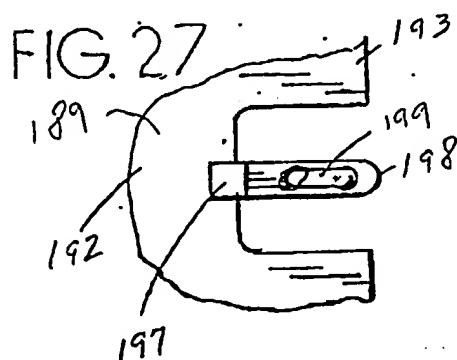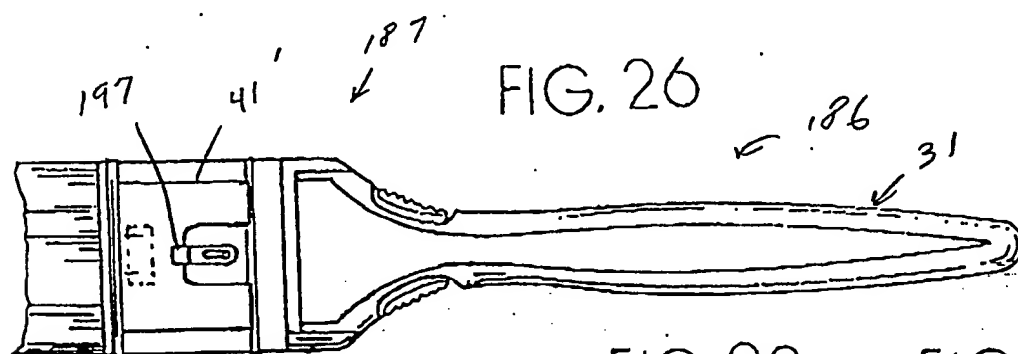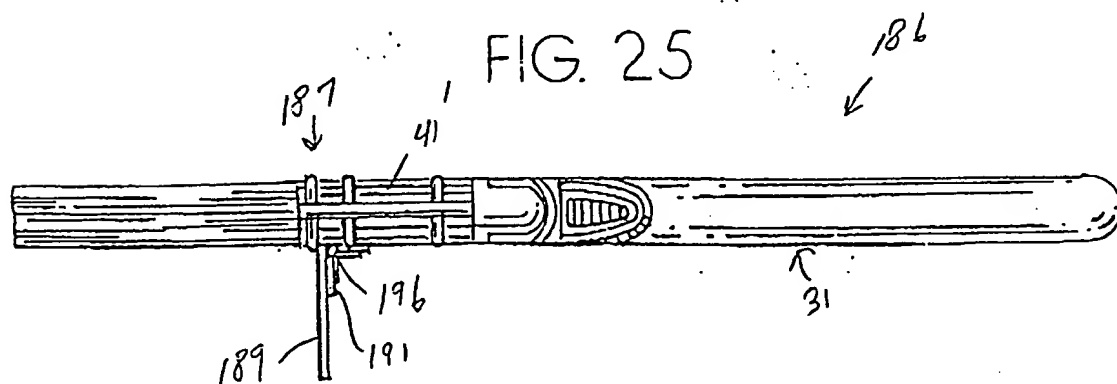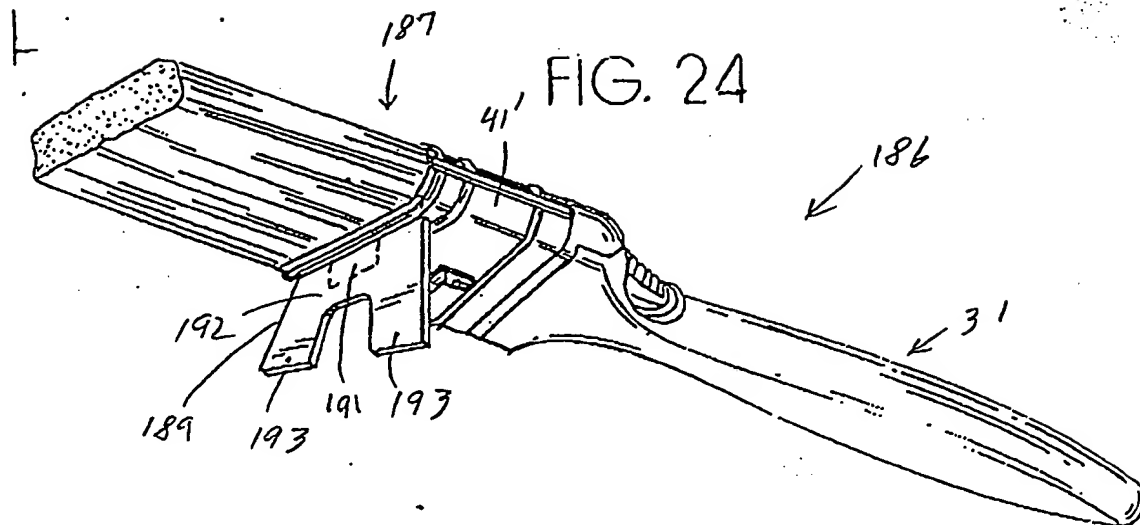

+

FIG. 30

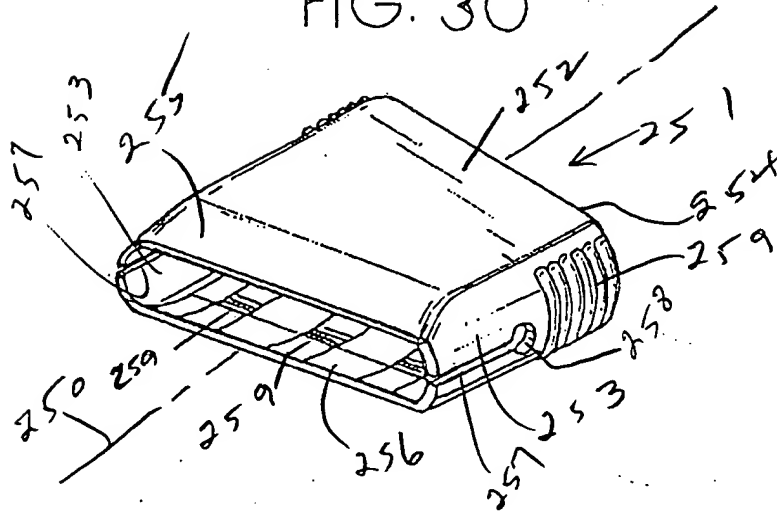


FIG. 31

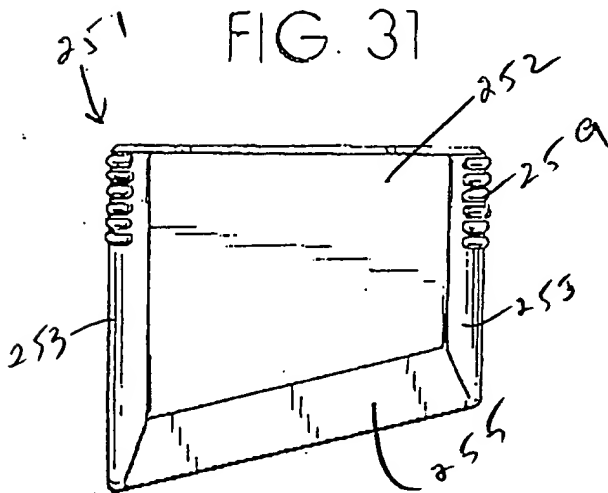


FIG. 32

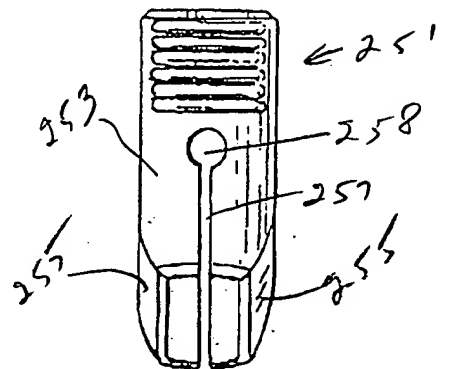


FIG. 36

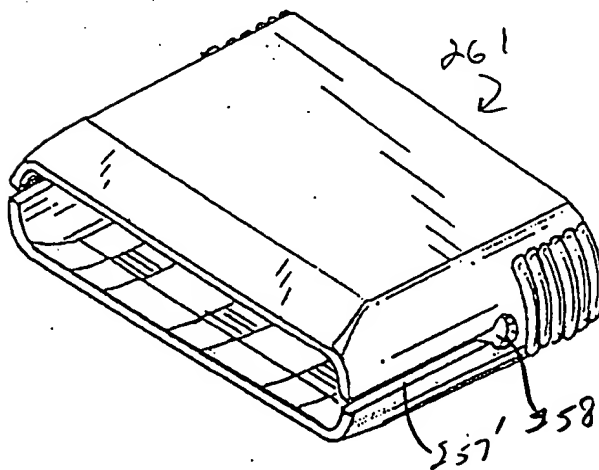
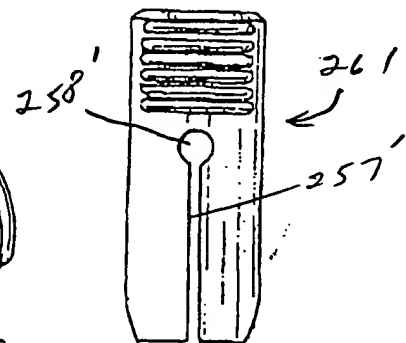


FIG. 37



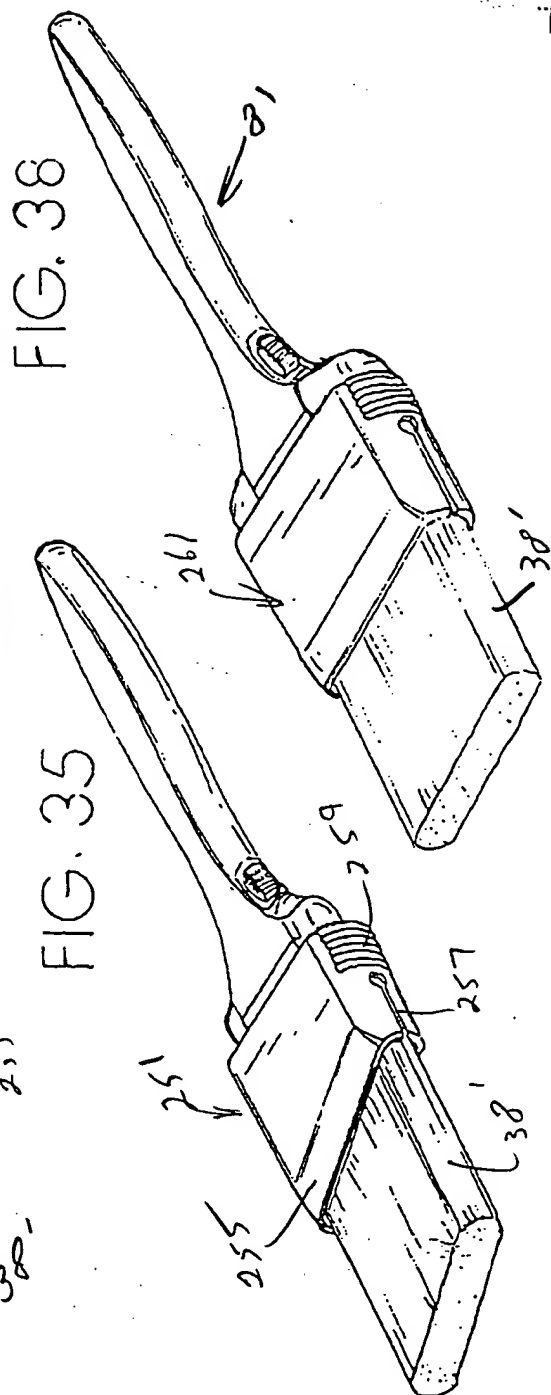
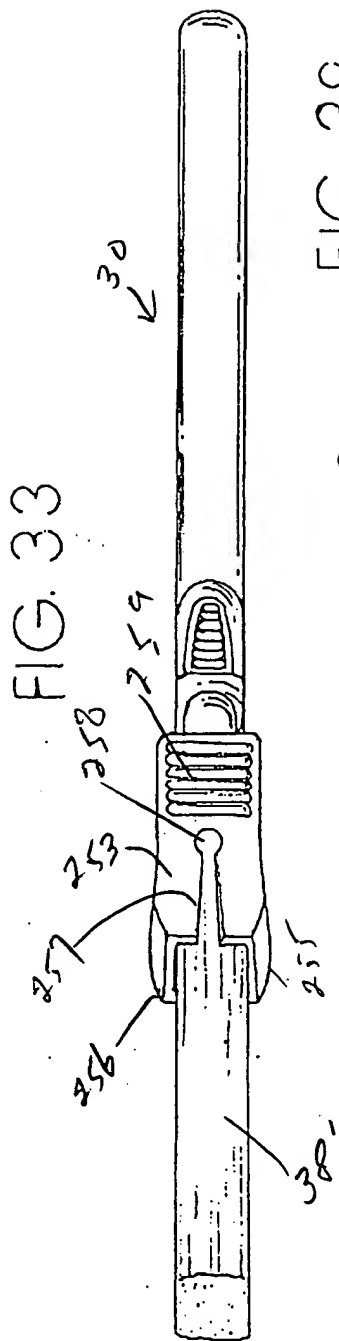
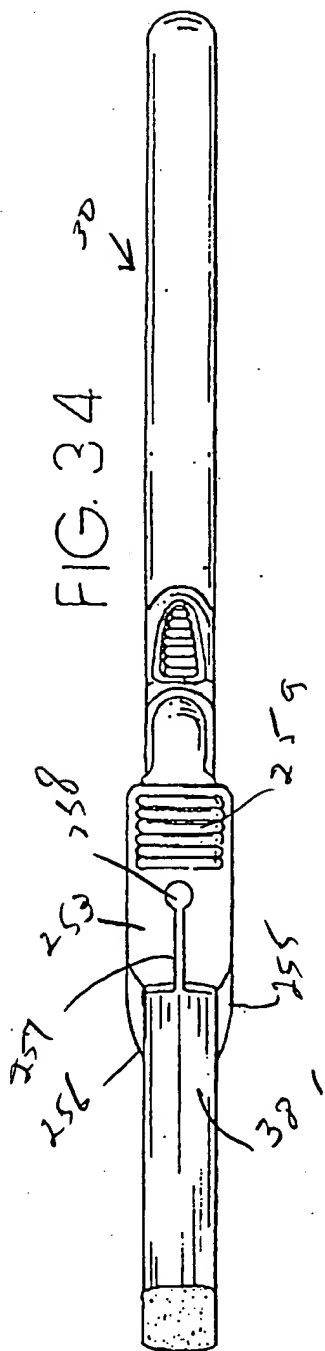


FIG. 39

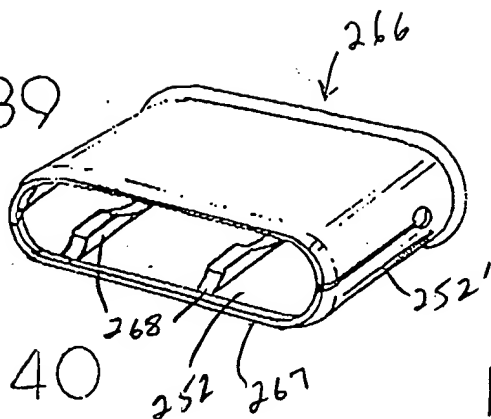


FIG. 40

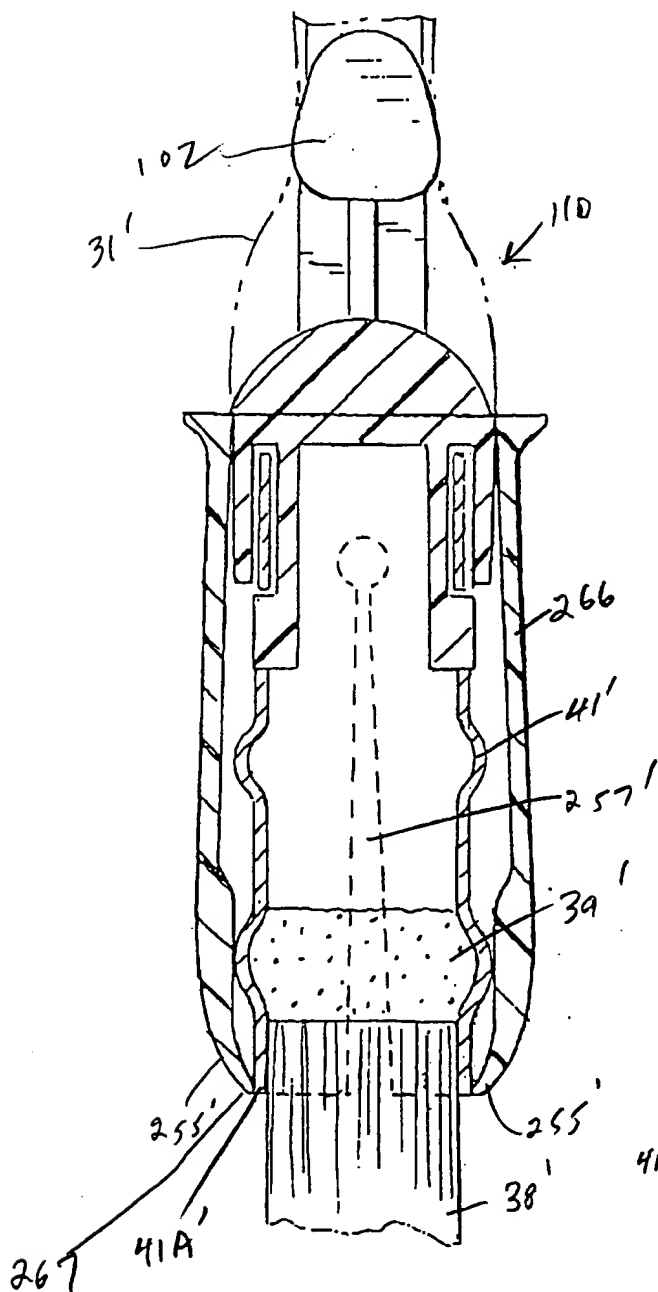
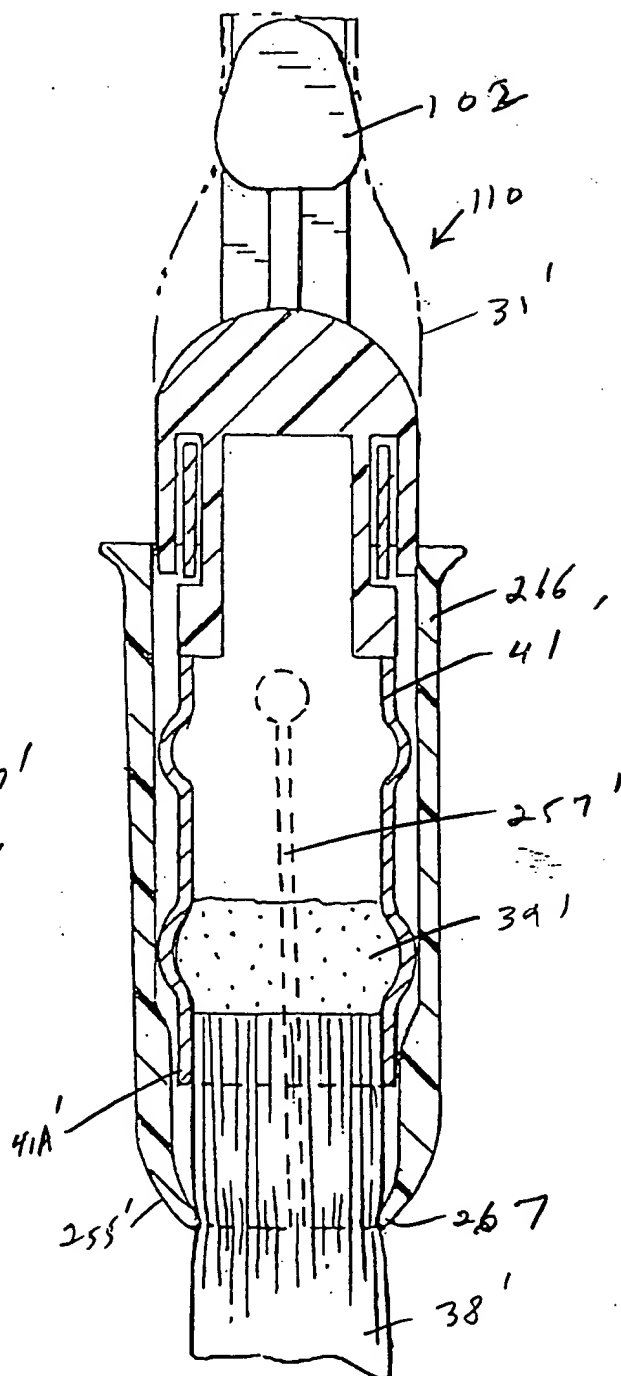


FIG. 41



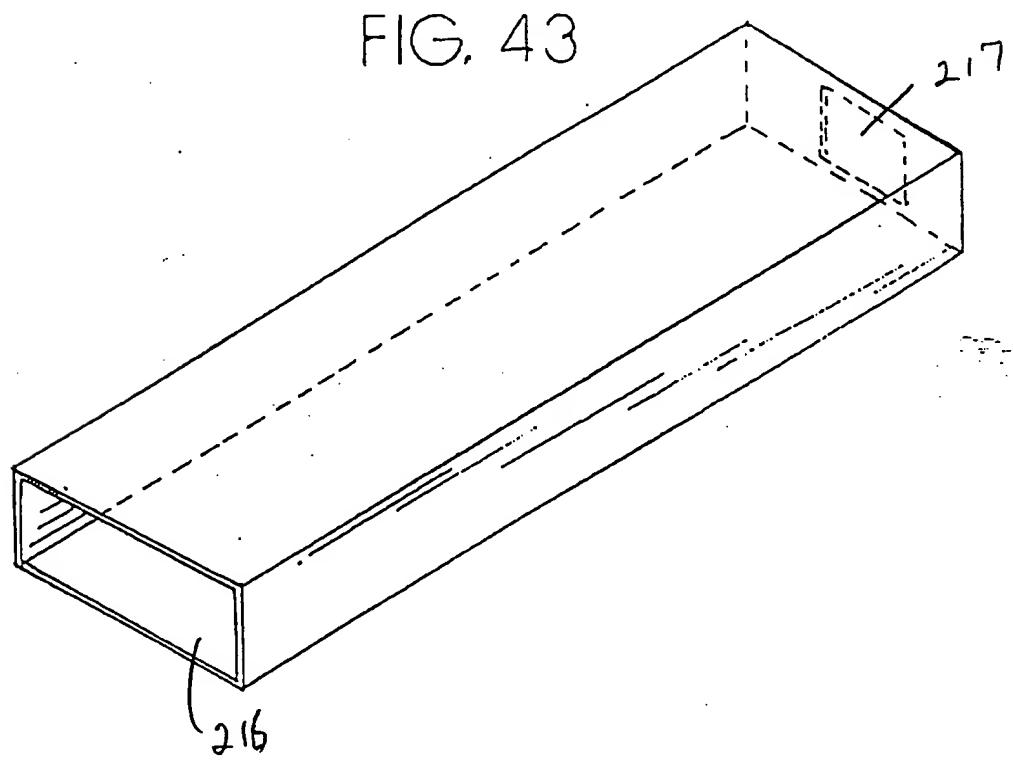
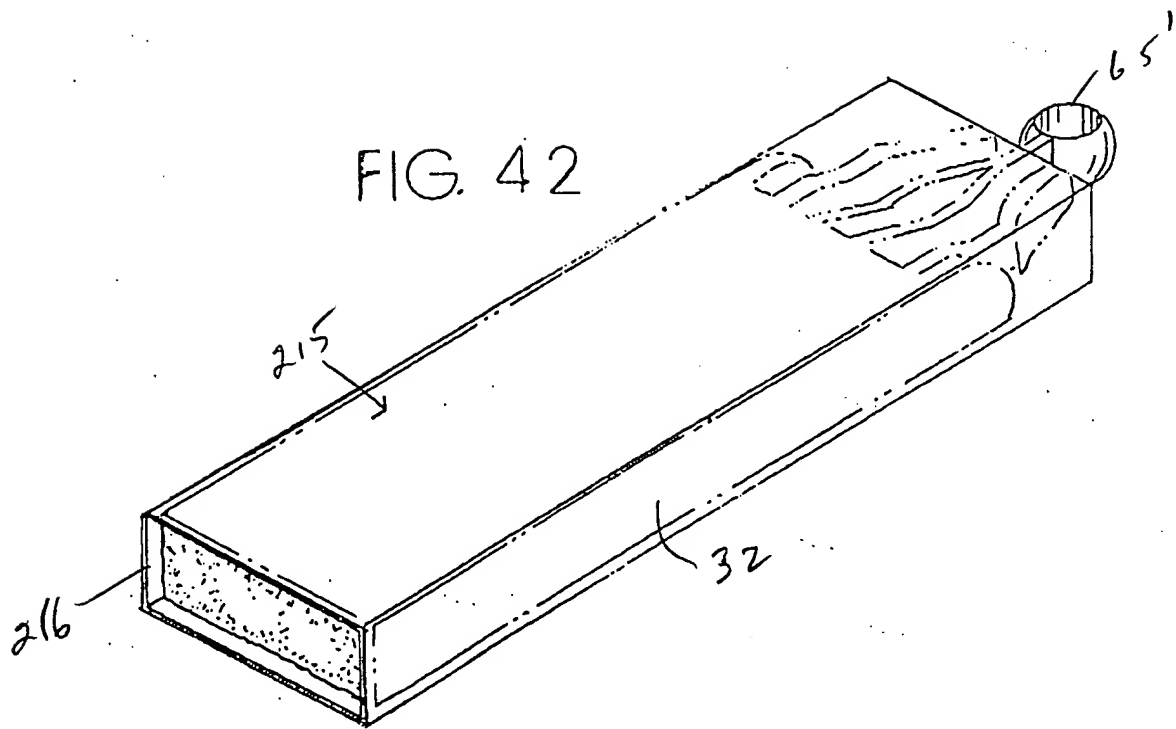


FIG. 44

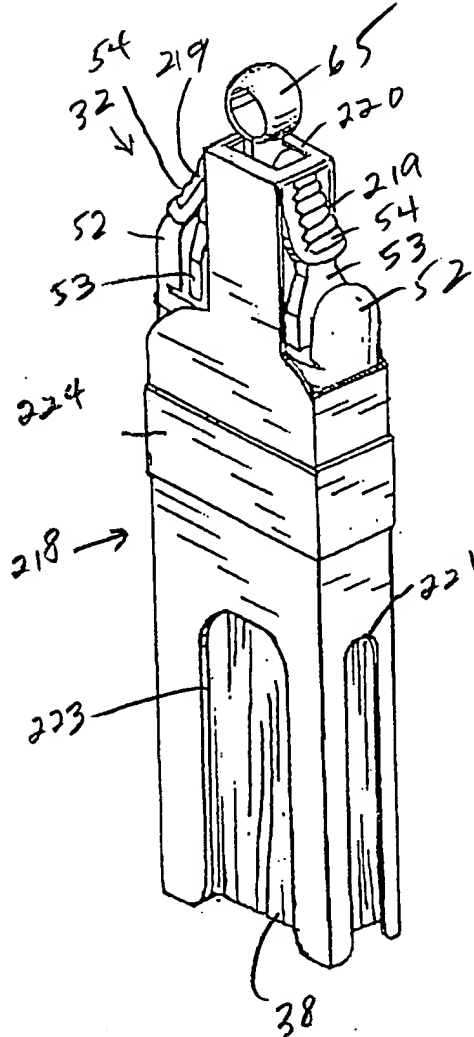


FIG. 46

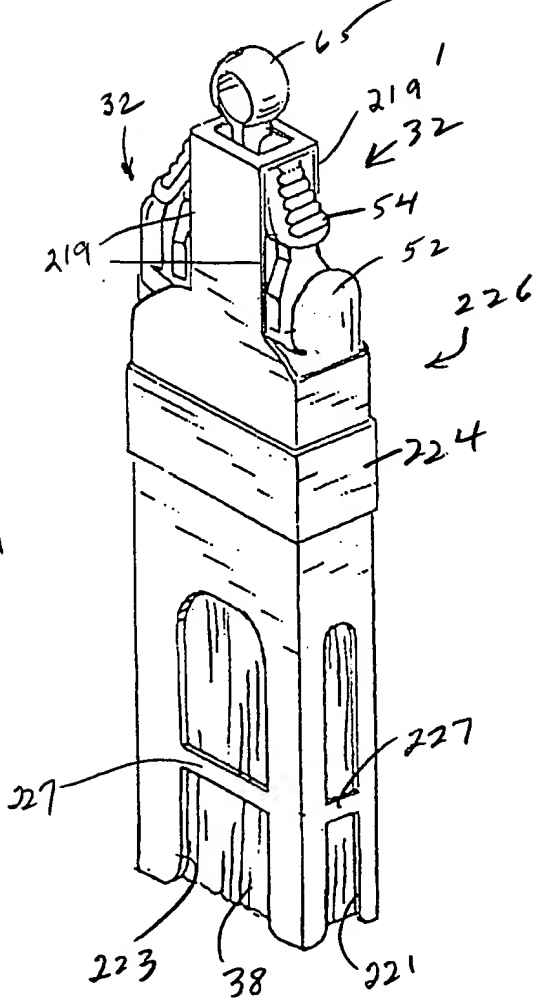


FIG. 45

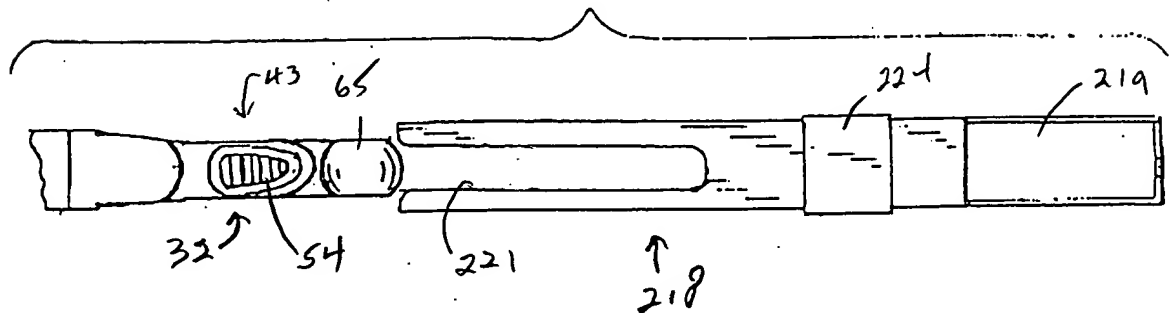


FIG. 47

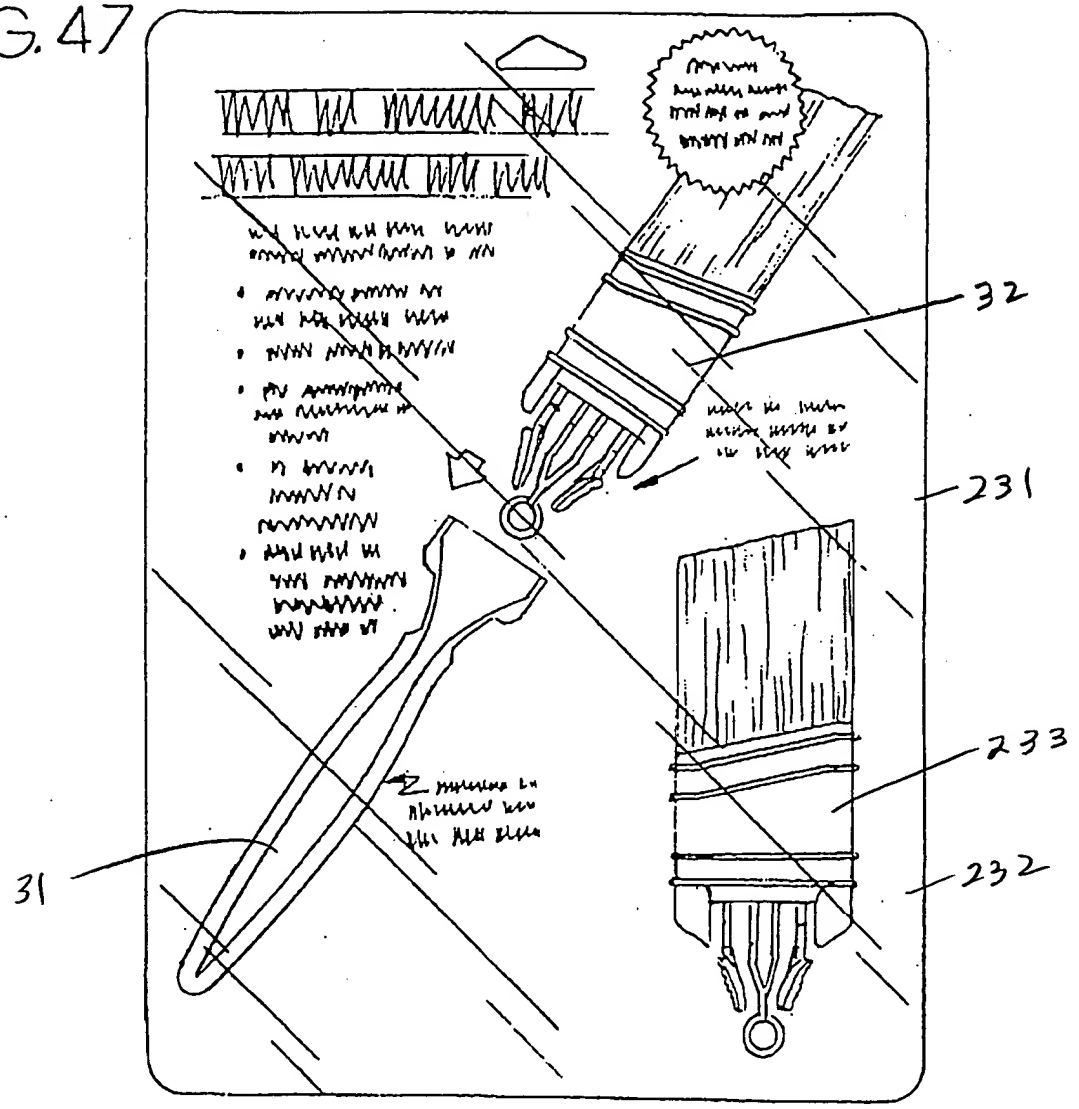


FIG. 48

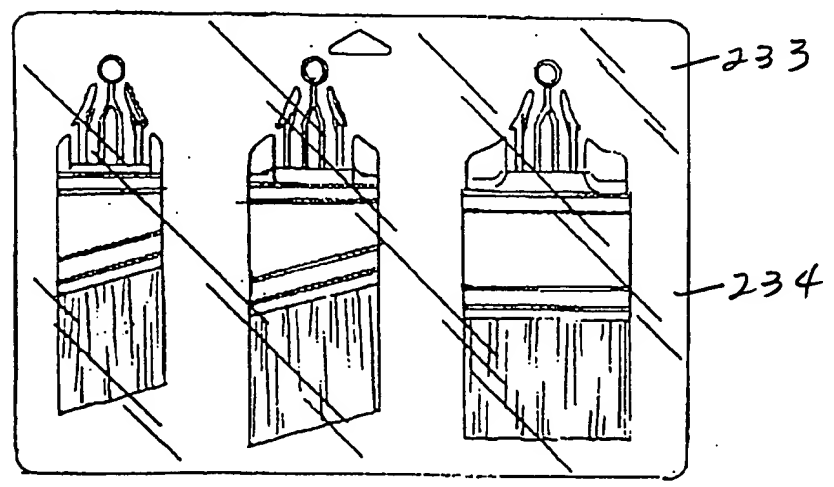


FIG. 49

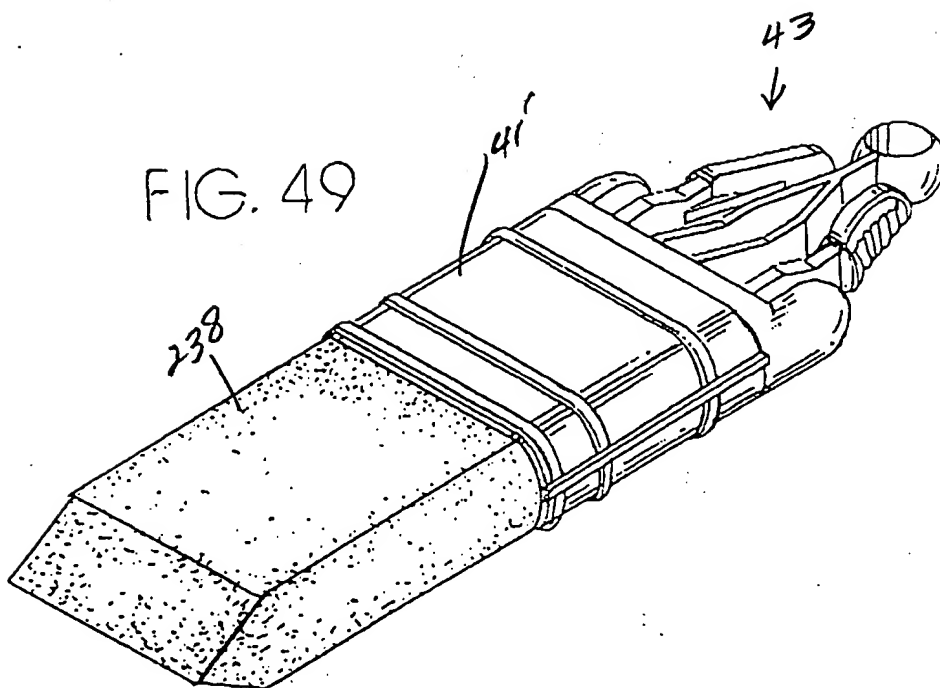


FIG. 50

